

d g s

DATA
GRAPH
SYSTEMS

INITIATE
(EVENT MARKER)

I 64
EVENT MARKER

64
ELECTRICAL
RECORDING

A-64
BLOOD PRESSURE

64
ELECTRICAL
RECORDING


4

3

2

1

PENS

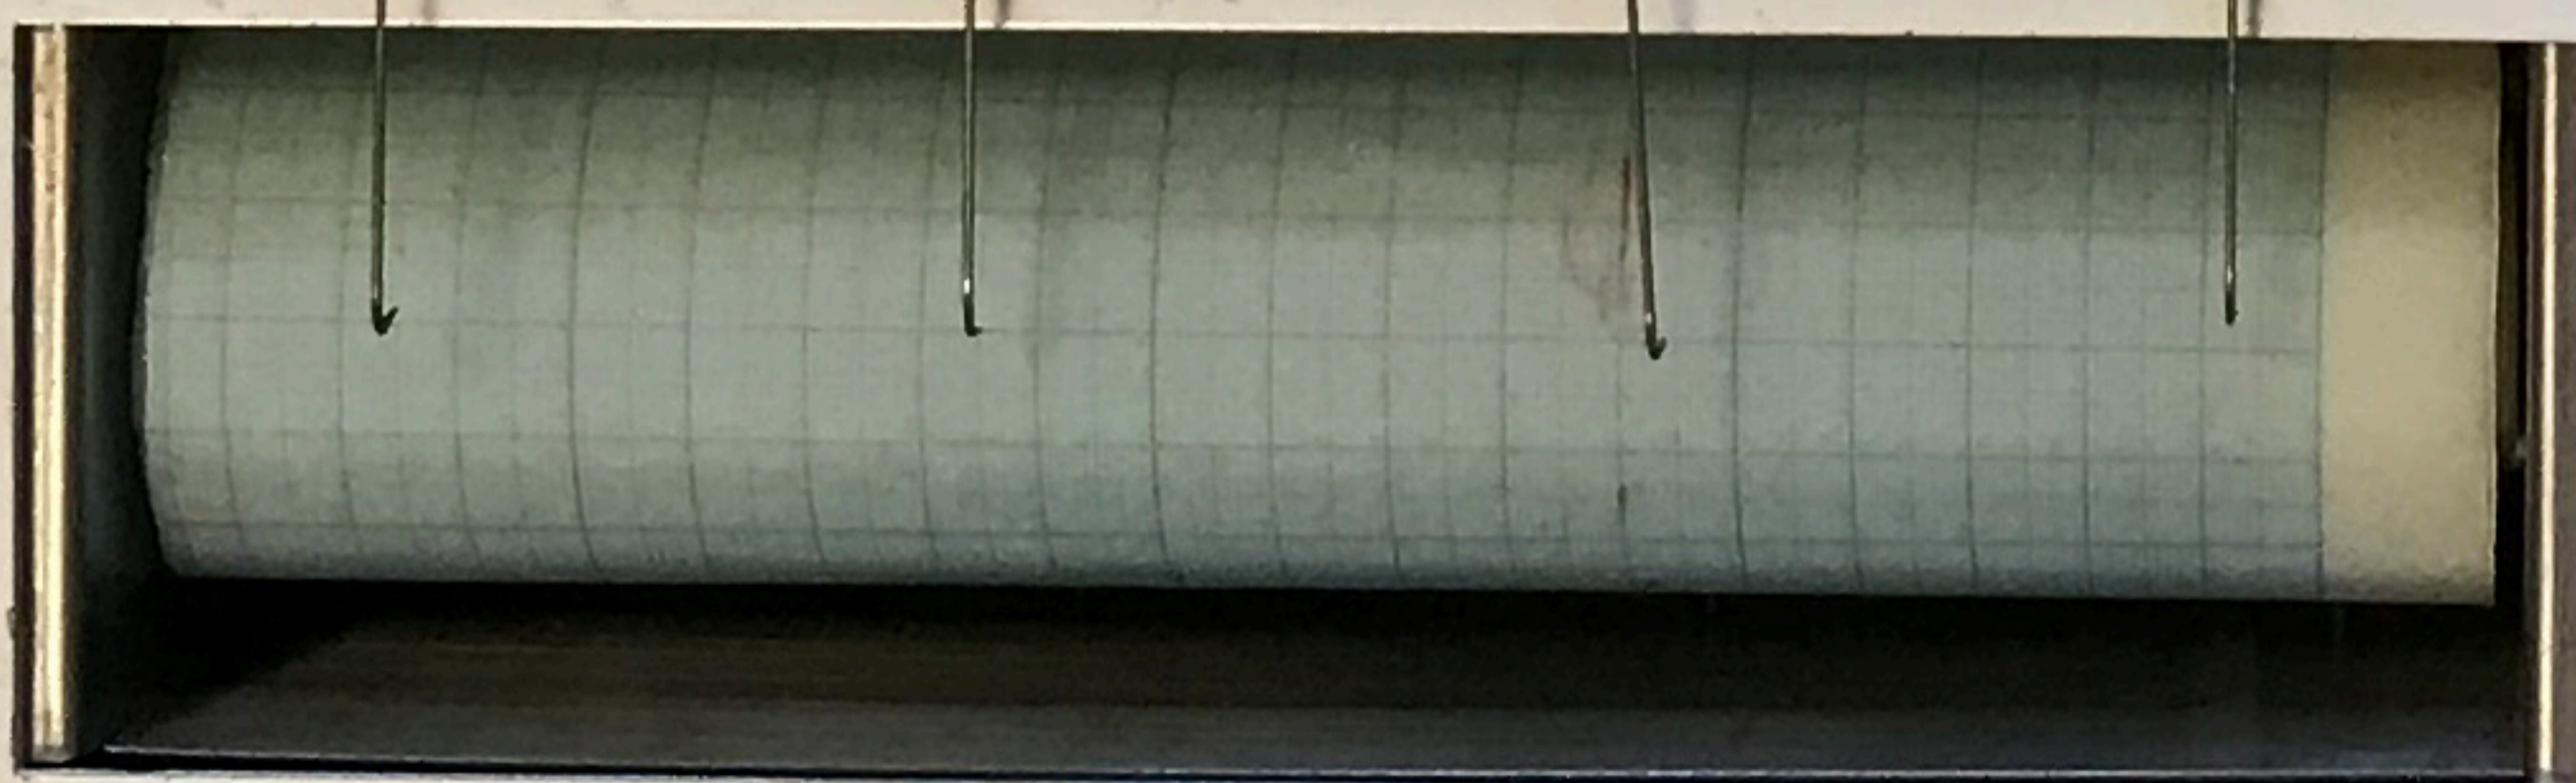

SUBJECT RESISTANCE

BALANCE

ON OFF

AMPLIFIER TWO

10K 400K 50K 350K 100K 300K 150K 200K 100K MAX

GSR H PLE INPUT

AC H DC

SENSITIVITY

3KΩ/mch

∞Ω

LAFAYETTE INSTRUMENT CO.
LAFAYETTE INDIANA

GSR 7601P

SUBJECT RESISTANCE

BALANCE

ON OFF

AMPLIFIER ONE

10K 400K 50K 350K 100K 300K 150K 200K 100K MAX

GSR H PLE INPUT

AC H DC

SENSITIVITY

3KΩ/mch

∞Ω

LAFAYETTE INSTRUMENT CO.
LAFAYETTE INDIANA

GSR 7601P

1/4 AMP SB



LAFAYETTE INSTRUMENT CO.
LAFAYETTE, INDIANA

6 OFF

INCHES/MINUTE

LAFAYETTE INSTRUMENT CO.
LAFAYETTE, INDIANA

76012